

# REPLACEMENT SHEET

Method for Increasing Capacity in an Automatic  
Clinical Analyzer by Using Modular Reagent Delivery Means  
Mizzer et al. / DCS-9129

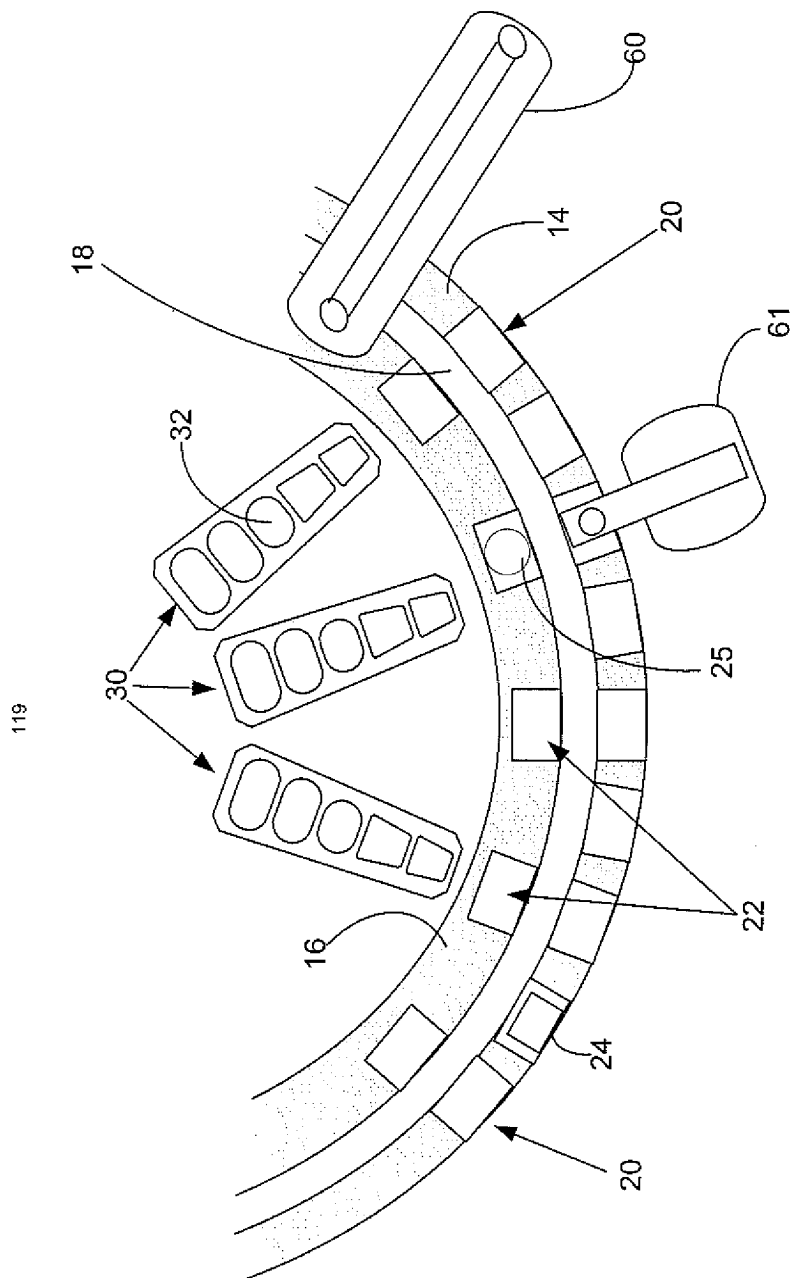


Fig. 2 PRIOR ART